


Instrumentation Conditions

- GC: Agilent 7890 w/ FID
- Cat no: 6225-6014 60m x 0.25mm x 1.4um
- Oven: 40 °C (15min) 10 °C /min 170 °C (1min)
- Carrier: Hydrogen, column flow 1.5ml/min
- Inlet: Split, 260 °C, split ratio 10:1
- Detector: FID 280 °C
- Samples: <20ppm Ethanol, Acetone, IPA, Acetonitrile, DCM and MEK, ETAC in Methanol
- Inject volume: 1ul

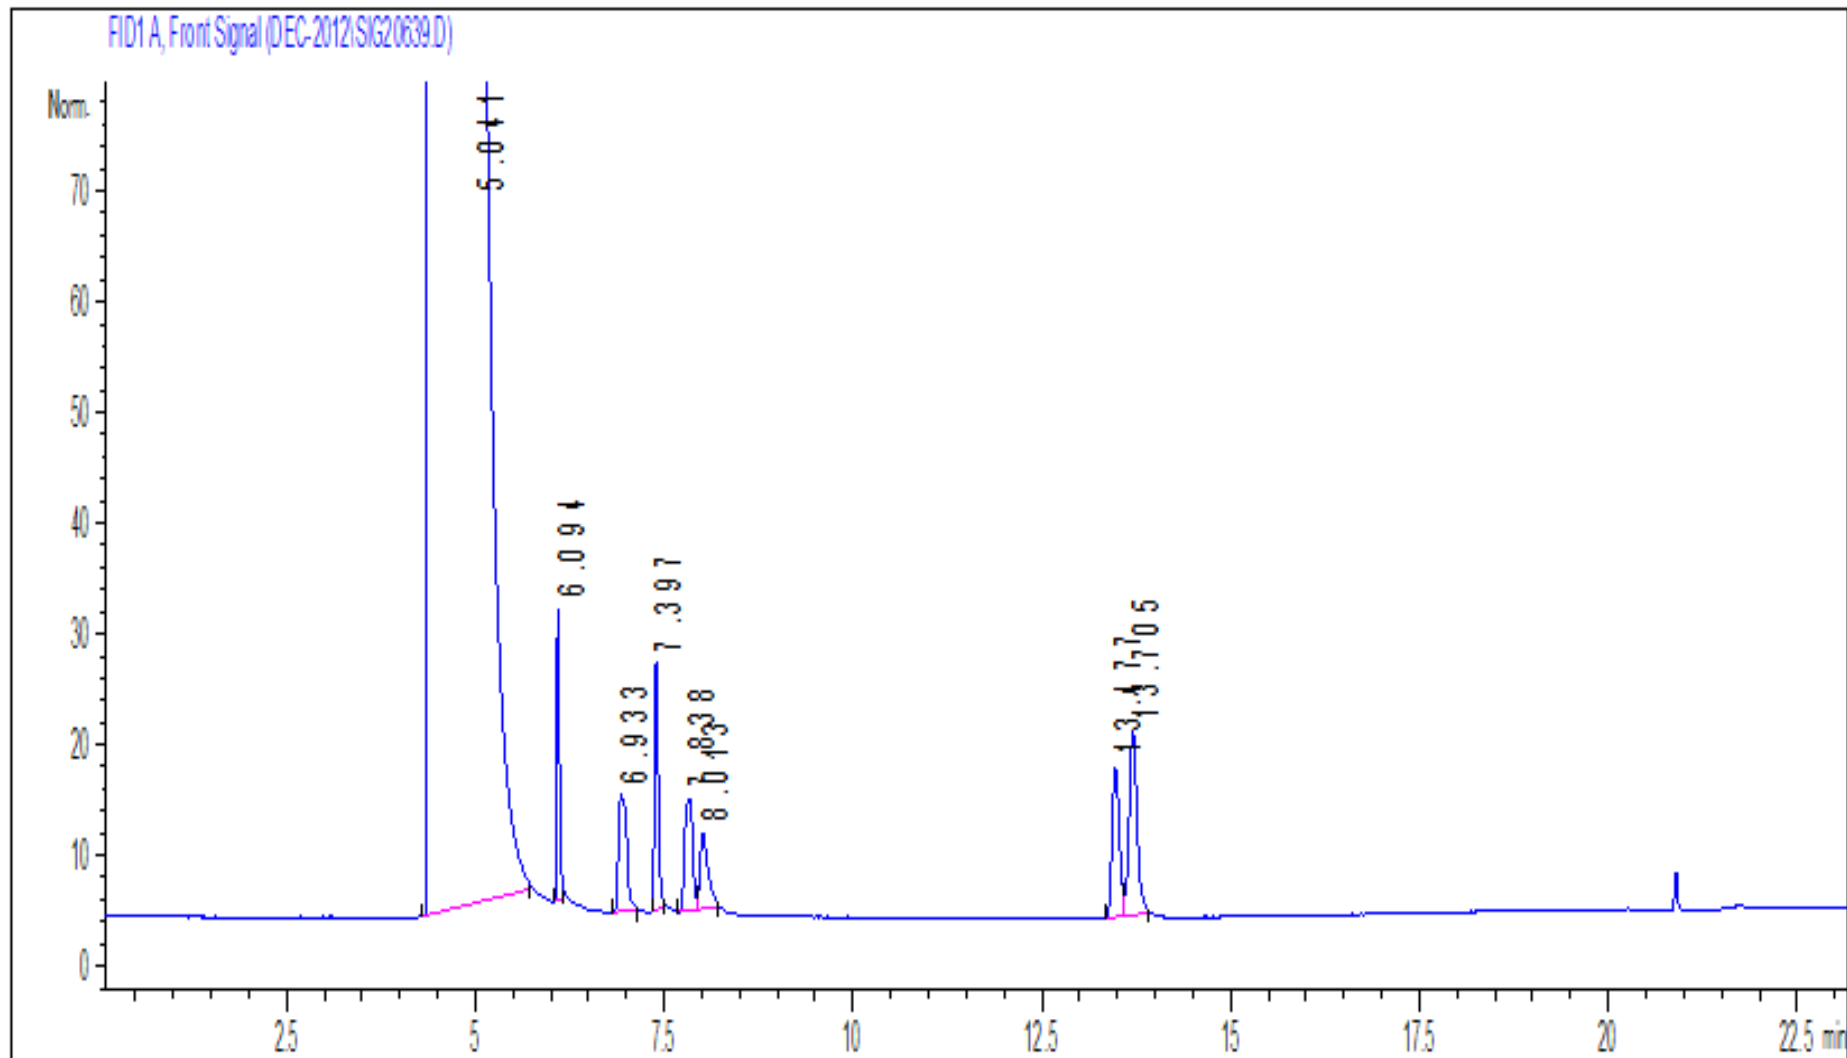

Peak Identifications and Resolutions

Peak	Compound	Concentration	Retention Time	Resolution
1	Methanol	Solvent	5.04	
2	Ethanol	10ppm	6.09	
3	Acetone	10ppm	6.93	
4	Isopropanol	10ppm	7.40	
5	Acetonitrile	10ppm	7.84	
6	Dichloromethane	10ppm	8.01	1.72
7	2-Butanone	10ppm	13.48	
8	Ethyl Acetate	10ppm	13.71	2.06